



Leak Testing for Biopharmaceutical Applications



PORTABLE HELIUM LEAK DETECTOR FOR BIOPHARMACEUTICAL APPLICATIONS

The Measure of Confidence



Agilent Technologies

Agilent Portable Helium Leak Detector prevents Product Loss



Introduction

The biopharmaceutical industry uses fermenter and bioreactor vessels to produce a myriad of products. These vessels can be quite large and typically have many wall penetrations. The penetrations can include stirrers, process instrumentation, vents, and fill and drain connections. Between process runs, the vessels are commonly drained, then steamed out before being “buttoned up” for the next campaign.

Infinitesimal leaks can be created during the cleaning process when valves are operated, and/or clamp fittings are opened and closed. In addition, as valves and other seals wear over time, they can develop leaks. Small leak paths will allow bacteria to enter the vessel, and ruin the process run.



Traditional Methods of Leak Detection

The biopharmaceutical industry has traditionally used pressure decay and/or visual (bubble testing) leak detection methods (such as the use of “Snoop®”) to detect leaks in process vessels. Both leak detection methods present major drawbacks:

- **Pressure Decay** uses compressed air to elevate the vessel pressure, and then relies on the ability of an operator to discern a change (decay) on a pressure gauge reading over a set period of time. **Furthermore, pressure decay just indicates that there is a leak, but does not pinpoint where the leak has to be repaired!**
- **Bubble Testing** uses a solution of soap and water squirted over various vessel penetrations, in an effort to identify leaks by seeing bubble formation at the leak site.



While the bubble test method can find larger leaks, it is a crude, highly subjective method of leak detection, often not repeatable.

Bubble testing cannot show small leaks or leaks in places like internal valve seals (valves are often installed in a horizontal position, and would have to be flooded with the soap solution in order to show the leak).



Agilent PHD-4, the solution...

What it is...

Agilent Technologies' PHD-4 is a portable leak indicator, which detects helium tracer gas that has been injected into the vessel, as it escapes the vessel through a leak path. The sensitivity of the PHD-4 in finding leaks is about **three orders** of magnitude greater than conventional bubble testing methods.

Why helium as a tracer gas...

Helium is present in only small amounts (5 ppm) in the ambient air. This results in low background noise and makes helium a very attractive gas for leak detection applications.

In addition, helium is:

- readily available on a worldwide basis.
- not toxic or flammable
- an inert gas.

Helium can be easily obtained in cylinders of various sizes and only needs to be of welding-grade purity.

The application...

The vessel is typically pressurized to about 2 atmospheres (absolute), at a 25% concentration of helium.

Testing can start immediately after pressurization. The operator moves the PHD-4 is flexible "sniffer" probe over suspected leak sites and into valve areas. The PHD-4 will provide both a visual (helium concentration) and audio (similar to a Geiger counter) indication of not only a leak, but the relative size and location of the leak found. The PHD-4 can measure concentrations generally down to as low as 2 ppm/helium, but practically, readings of 20 ppm and higher represent leaks that

PHD-4 - Principal of Operation

The object or vessel to be tested is filled with a helium-air mixture at a pressure level exceeding ambient conditions. The PHD-4 probe is then passed over the suspected leak area(s), and a gas sample is continuously drawn through a flexible hose by the PHD-4 sampling pump. This pump pulls the gas sample over a special silica capillary which blocks atmospheric gases but allows helium molecules to permeate into the sensor (ion pump based) because of their small size. The sensor output signal indicating the helium presence is processed by dedicated software and allows a direct read-out of helium concentration on the display.



can be repaired, prior to returning the process vessel to service.

What is the pay back

Experience with the PHD-4 in this industry over the last three years has confirmed its ability in finding small leaks, until now undetectable with "Snoop®" or pressure decay methods. PHD-4 has helped to virtually eliminate lost product due to bacteria entering through undiscovered leaks in the process. The leak testing time is drastically cut, and the probability of identifying important leaks is greatly enhanced. Generally the value of the first batch of product saved using the PHD-4, will pay for its cost many times over.

Comparison and Conclusion

The PHD-4 can be viewed as a qualitative and quantitative tool, similar to "Snoop®", but 1000 times more sensitive than "Snoop®" in finding leaks.

Engineers from a large U.S. pharmaceutical company using the PHD-4 have called it the "best practices" method for finding leaks in bioreactors and fermenters.

Reactor and fermenter vessels require more rigorous ways to find and eliminate leaks than the widely-used pressure decay and/or Snoop® methods. Agilent Technologies' PHD-4 portable helium leak detector offers the solution.




PHD-4 Display

Portable Helium Leak Detector

AGILENT PHD-4 - FEATURES AND BENEFITS

High Selectivity	PHD-4 is sensitive only to helium. There are no false signals due to the presence of any other gases.
High Sensitivity	PHD-4 is nearly as sensitive to small leaks as a more expensive mass spectrometer leak detector used in the sniffing mode. It will find the leaks in bioreactors and fermenters that need to be addressed.
Battery Operated	PHD-4 can be operated without a main power supply. Up to 4 hours on a single charge.
Simple Operation	PHD-4 is very easy to use and does not require any special operator training. All the active menus of the PHD-4 are available in four languages.
Very Low Maintenance	Replacement of sampling line filters is straightforward and requires only a screwdriver.
Portable	PHD-4 is lightweight, portable and easy to carry, even to the most difficult leak check locations. It weighs only 2.6 kg.

OUTLINE DRAWING

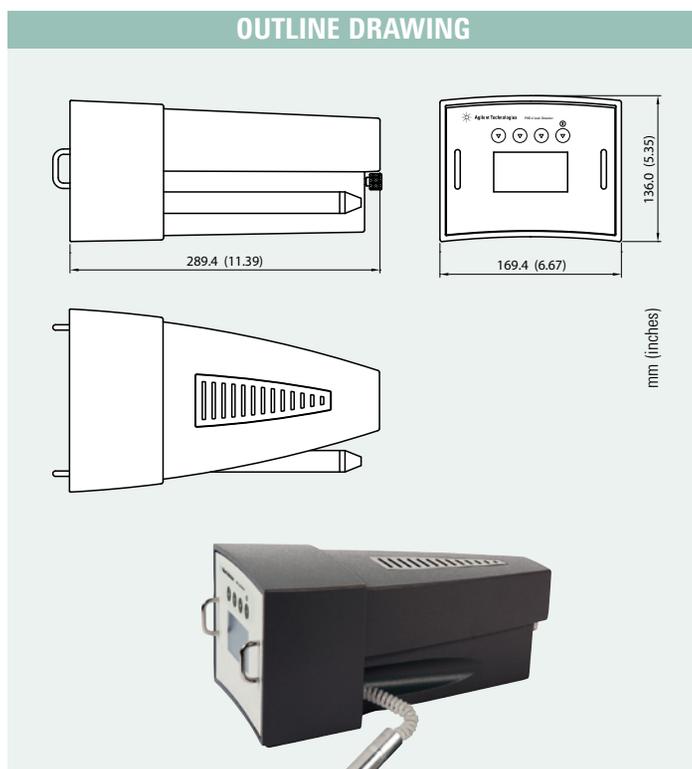

AGILENT PHD-4 - TECHNICAL SPECIFICATION

Lowest Detectable Helium Concentration:	2 ppm (parts per million)
Lowest Detectable Helium leak:	5 x 10 ⁻⁶ atm cc/s 5 x 10 ⁻⁶ mbar l/s 5 x 10 ⁻⁷ pa m ³ /s
Response Time:	< 2 sec
Recovery Time:	<10 sec (from 50 ppm to 0 ppm)
Start up time, including self check-up:	3 min approx.
Electrical Supply:	Rechargeable Battery included Power Supply included 110-240 V 50-60 Hz
Battery operation Time:	4 hours
Maximum Signal Drift:	10 ppm/10 min
Operating Conditions	Temperature: +5°C to +35°C Humidity: 90% maximum relative humidity
Storage Conditions	Temperature: -20°C to +60°C Weight: 2,6 Kg (5.7 lbs)
Compliance to Norms:	CE, CSA/UL approved

United States and Canada

Agilent Technologies
121 Hartwell Avenue
Lexington MA 02421 USA
Toll free: +1 800 882 7426
vpl-customerservice@agilent.com

Europe and Other Countries

Agilent Technologies Italia S.p.A.
via F.lli Varian 54
10040 Leini, (Torino) Italy
Toll free: 00 800 234 234 00
vpt.sales@agilent.com
vpt-customerservice@agilent.com

This information is subject to change without notice

© Agilent Technologies, Inc. 2012
Published June 30, 2012
VPD-0212EN



Agilent Technologies